

User Manual

NanoVi™ Devices

Eng3 Corporation

eng3

Life Science Technology

NanoVi Eco™ / NanoVi Pro™ / NanoVi Exo™



User Manual

User Manual Eng3 Part Number: 4530-00

M004-rev07

Table of Contents

1	Device Description	1
2	Contra Indications	3
3	Possible Side Effects	3
4	Warnings and Precautions	4
5	Initial Set Up	4
	5.1 Unpacking Device & Accessories	4
	5.2 Set Up	5
6	Operating Instructions	7
	6.1 Use of Flex-Arm	7
	6.2 Nasal Cannula	7
	6.3 Power On	8
	6.4 Touch Screen Interface	8
	6.5 Application Schedule	8
	6.6 Lights Illuminating the Glass Container	9
	6.7 Session Running	9
7	Operating in Standard Mode	10
8	Operating in SmartCard Mode	12
	8.1 Owner Card	12
	8.2 User Card	15
9	Use with Accessories	17
	9.1 Transportation Case	17
10	Cleaning Instructions	19
11	Maintenance	20
12	Storage	20
13	Troubleshooting	21
	13.1 Normal Operation	21
	13.2 Errors	21
14	Product Specifications and Registrations	23
	14.1 Technical Specifications	23
	14.2 Product Registrations	24
15	Warranty	25
16	Service Policy	26
17	Ordering Parts and Accessories	26
18	Contact Information	27

1 Device Description

The process that takes place within the NanoVi™ device occurs in four steps:

- 1 Creation of a constant air stream with intake of ambient air
- 2 Humidification of the air stream, enriching the air stream with water molecules
- 3 Generation of a specific signal known to initiate repair mechanisms in the body
- 4 Transfer of the signal across the humid air stream to the user via a Flex-Arm.

The NanoVi device is designed to help initiate the body's natural repair of free radical damage. When this damage accumulates it is called oxidative stress damage and is, in optimal situations, counterbalanced by the body's oxidative response. This involves repair and rejuvenation at the cellular level. Within the body, on an ongoing basis, oxidative response is triggered by a specific signal naturally emitted by certain free radicals (called Reactive Oxygen Species or ROS). NanoVi™ devices generate the same specific signal, which is transferred across a humid air stream to the user.

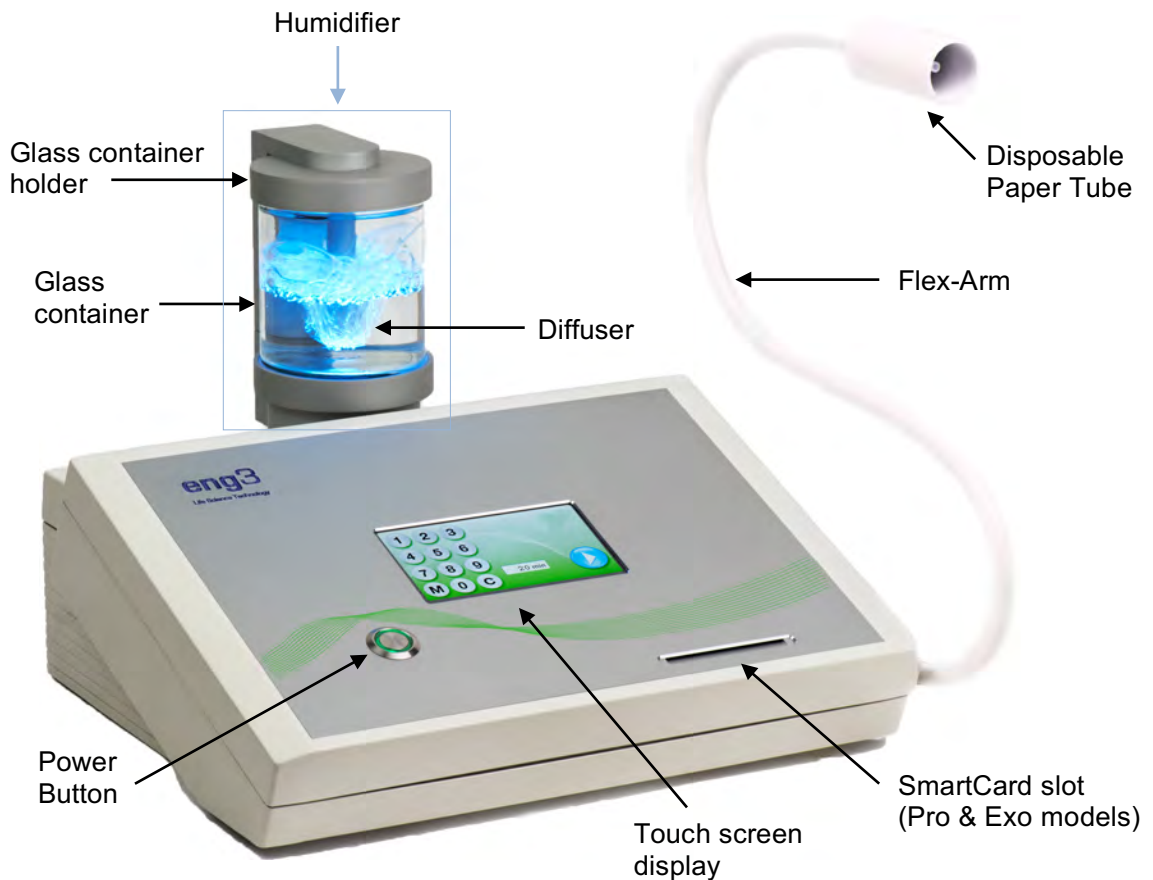


Figure 1.1: Front view of the NanoVi Exo™ device

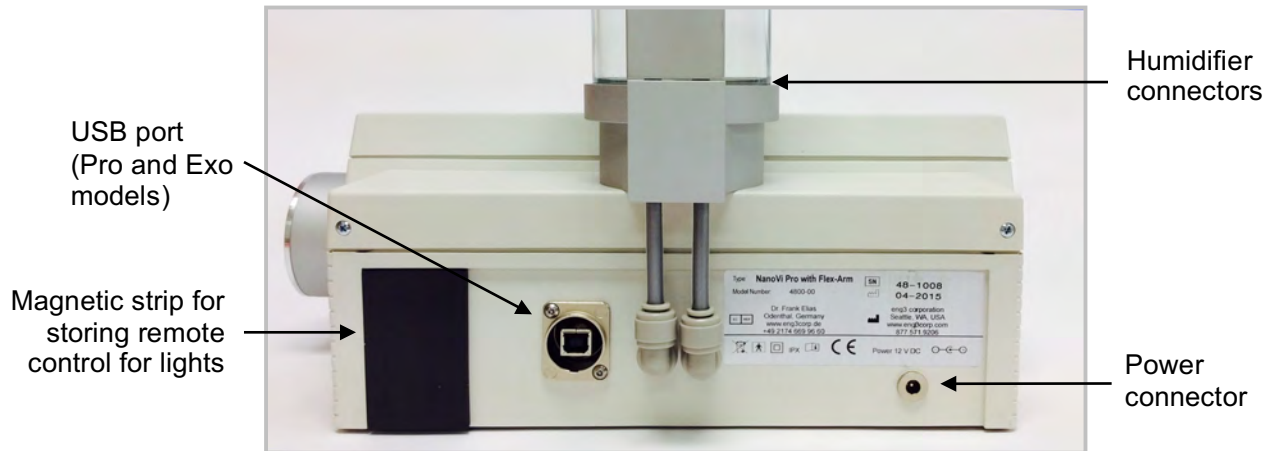


Figure 1.2: Back view of the NanoVi™ device

The NanoVi™ device has a universal power supply and is plugged into a standard power outlet, 110v to 220v.



Figure 1.3: Power supply and power cord

2 Contra Indications

To date, no contra indications are known.

Patients and pregnant women should consult their physician before using the device. This is a precaution to prevent possible adverse reactions that are as yet unknown.

3 Possible Side Effects

The following temporary reactions have been occasionally observed when first using the NanoVi™ device. Typically, when side effects occur the body is going through a detoxification process and the session time was too long.

- Drowsiness: Use a shorter session length for the first few sessions, Choose the time of the first session to accommodate unexpected drowsiness, which might occur after the initial application. This will disappear after several sessions.
- Insomnia: To avoid trouble falling asleep, do your session at least 4 hours before going to bed when you first start using the device.
- Dizziness and/or headaches: Dizziness and/or headaches can temporarily appear and will disappear after a short period of time. Should this occur, use shorter session times.
- Changes in stool: If unwanted changes in stool consistency appear, use shorter session times.
- Skin reactions: If skin reactions, such as reddening and itching, appear use shorter session times until skin reactions have disappeared.

4 Warnings and Precautions

Read the User Manual carefully before using the NanoVi™ device for the first time.

- Refer to the User Manual whenever questions or uncertainties arise with respect to correct handling of the NanoVi™ device.
- Always use the original power supply (power adapter). Operation is restricted to 12V DC at the device input. Contact your retailer if the original power adapter is defective or lost.
- Before use, make sure that the water level in the container is between the maximum and minimum levels marked on the container. Never fill above the maximum level as a higher level could cause water drops to form in the tubes.
- Change the water in the glass container regularly. At least once a day if there are multiple users and at least once a week or every five hours of use for individual users. Use only distilled, purified or osmotic water. Normal water could cause chalky deposits in the diffuser and the glass container.
- Never use the device if any part of the humidifier is damaged. A defect can cause leakage and penetration of water into the inner parts of the device. Contact your retailer to purchase a replacement.
- Protect the NanoVi™ device from extreme temperatures and moisture during operation or storage. These conditions can damage internal components.
- The device should only be used on a stable surface. The NanoVi™ device should not be used during transport.

5 Initial Set Up

5.1 Unpacking Device & Accessories

1. Inspect shipping box for damage upon arrival. Contact your retailer immediately if box is damaged.
2. Unwrap the NanoVi™ device carefully and keep the original packing materials for future transportation of the device.

3. Place the NanoVi™ device on a flat, clean surface, such as a table.
4. Unpack all accessories and place them beside the device.

5.2 Set Up

There are no special tools or materials required for setup other than distilled, purified or osmotic water to clean and fill the glass container.

Follow these steps to set up your device:

1. Place the NanoVi™ device on a clean, solid surface
2. Rinse glass container using distilled, purified or osmotic water.
3. Fill the container with distilled, purified or osmotic water. Make sure the water is between the maximum and minimum filling levels on the container.



WARNING: Do not fill the container with more water than the maximum filling level indicates, as water drops or water may enter the tube system or device.



WARNING: Fill water at least to the minimum filling level as indicated on the container. Adequate air humidification depends on the amount of available water.

4. Hand tighten glass container firmly into the glass container holder.
5. Insert humidifier into the fitting on the top of the device, at the back. The connecting tubes protruding from the humidifier slide down into the device as shown in Figure 5.1. There will be a small gap between the humidifier and the device when there is a proper connection.

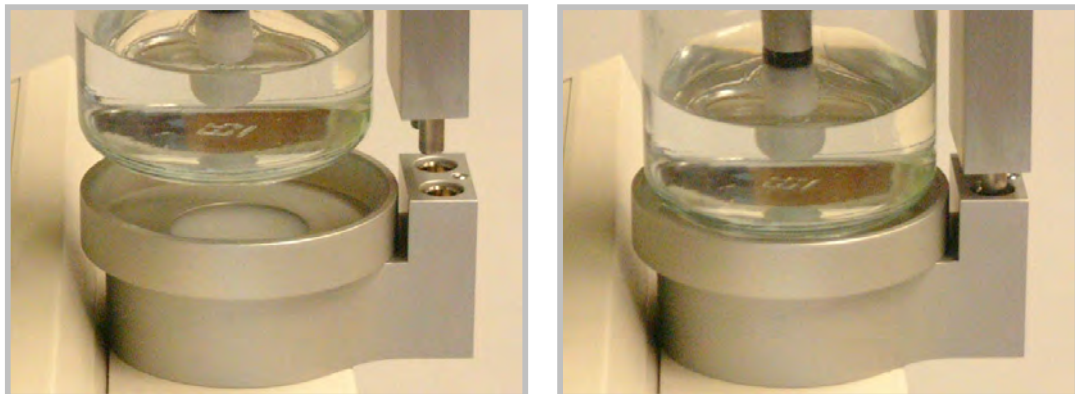


Figure 5.1: Inserting humidifier into device

Confirm that there is only a small gap between the humidifier and the device. This ensures a proper connection. (Figure 5.2).

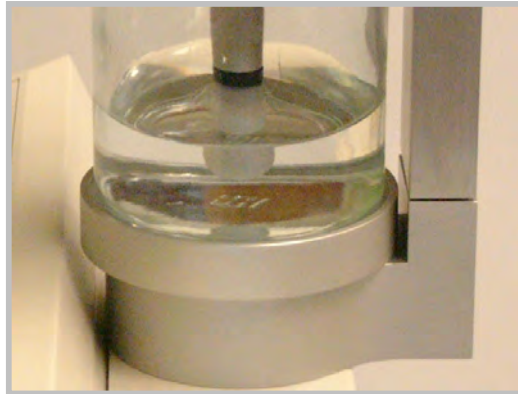


Figure 5.2: Correct insertion of humidifier



WARNING: Do not force humidifier into the device; it will fit firmly with a small gap between the two metal pieces.

6. Connect the power cord to the power supply. Plug the power supply into the NanoVi™ device. Note Figure 1.2 to locate the power connector on the back of the device. Plug the power cord into an electrical outlet.

The NanoVi™ device is now ready for operation.

6 Operating Instructions

6.1 Use of Flex-Arm

NanoVi devices come with an installed Flex-Arm, as shown in Figure 6.1.

Remove the protective cap from the outlet on the Flex-Arm, if it is in place. Place one of the disposable paper tubes that come with the device onto the end of the arm and push it on to fit snugly.

Gently pull the Flex-Arm towards your face. The end of the paper tube should be in front of your nose, one to three inches away, as shown in Figure 6.2. The Flex-Arm can be moved and repositioned for comfort but must not be bent sharply. It is important to be sitting or lying still and to have the Flex-Arm correctly positioned so that you are inhaling the output from the device.



Figure 6.1: NanoVi Pro™ Device



Figure 6.2: Flex-Arm use



WARNING: Do not try to bend the Flex-Arm into sharp angles.

6.2 Nasal Cannula

The NanoVi device can be used with a nasal cannula inserted on the outlet in the middle of the Flex-Arm attachment. For proper operation, a short cannula that has one-foot instead of the standard seven-foot length tubing is used. The one-foot disposable cannula is shown in Figure 6.3. The user does not have to sit or lie still when using the cannula. It allows the user to make small movements and turn their head without interrupting their session. Use of the cannula is shown in Figure 6.4.

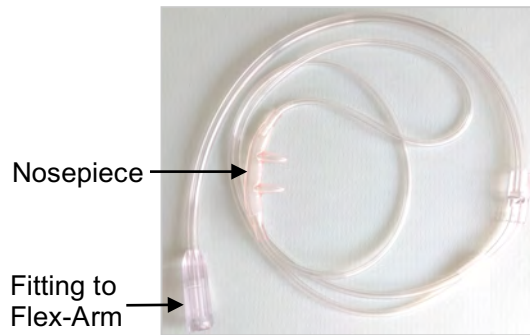


Figure 6.3: Nasal cannula



Figure 6.4: Nasal cannula use

6.3 Power On

Press the large button on the front of the device to turn the power on. The power button will illuminate with a green circle and the touch screen display will automatically start with a self-test. Once the device is ready, the screen will display standard user options. Pressing the power button at the end of a session will turn the device off. If you do not turn the device off and it is not used for 15 minutes, it will turn itself off.

6.4 Touch Screen Interface

The touch screen is operated by lightly touching it with a finger. If necessary, a soft blunt object could be used to operate the touch screen. Hard or sharp objects should never be used.

A tone sounds each time you press a button, indicating that your input was registered through the touch screen.



WARNING: The use of hard or sharp objects to operate the touch screen could result in damage to the device.

6.5 Application Schedule

The session time depends on which NanoVi™ device is used. The NanoVi Exo™ device is twice as powerful as the NanoVi Pro™, and the Pro device is twice as powerful as the NanoVi Eco™. As a

result, the standard session time of 15 minutes on the Exo is similar to 30 minutes on the Pro, or 60 minutes on the Eco device.

It may be necessary to build up use of the device slowly. The appropriate amount of time depends on the state of each person's health and physical condition. Although adverse reactions are experienced by only a small percentage of people, a safe approach is to start by using the NanoVi Eco™ device for only 10 minutes the first day (5 minutes for the NanoVi Pro™ or just a few minutes on the NanoVi Exo™). If you feel well and are not light headed, it is fine to do more time. Feeling light headed or uncomfortable in any way signifies that the session should be stopped for the day and time should be added gradually. If adverse reactions occur, revert to shorter session times.

It is important to start slowly to stay within your comfort zone. If you are highly sensitive and/or in need of detoxification, start with only a few minutes and keep adding time each day, as long as there are no adverse reactions. In the event of an adverse reaction, reduce the number of minutes of use until there is no reaction, then start adding minutes until the desired session time is reached.

For prevention in younger healthy people, two or three standard NanoVi™ sessions per week are adequate. Individuals that have health challenges, are older, or are performance athletes should use the device more. NanoVi™ devices can be used every day and several times a day, if desired. There is no potential to be harmed by the device so overuse is not a concern, once you are accustomed to it. The device can be used for many hours a day if desired.

6.6 Lights Illuminating the Glass Container

The lights illuminating the glass container are adjusted with a remote control. The remote control must be pointed at the water in the glass container and within about two feet to work.

The lights can be turned off or changed with the remote control.

The remote control attaches to the back of the device with Velcro for storage.

The remote control comes with a battery already inserted.

6.7 Session Running

When a session is started you will hear a quiet humming sound, see bubbles in the glass container, and, if the lights are turned on, see the illumination of the water in the glass container.

If the water is bubbling, the device is operating correctly. If it is not bubbling, check to make sure the humidifier is correctly seated in the back of the device and that the glass container is firmly screwed into the glass container holder.

7 Operating in Standard Mode

All three NanoVi™ devices can be operated in standard mode. Once the device is turned on, a splash screen appears. A self-test runs for 10 seconds with progress shown by the bar at the bottom of the screen. (Figure 7.1)

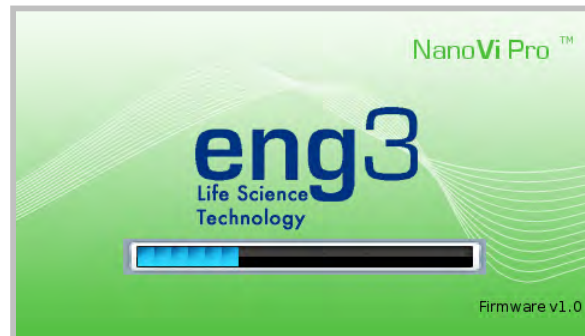


Figure 7.1: Initial splash screen

Upon completion of the self-test, an input screen appears allowing you to enter the amount of time for the session (Figure 7.2). Enter the desired session time by touching the appropriate numbers on the touch screen. Time is entered in minutes. The minutes entered shows in the session time indicator in the centre of the screen. Touching the “C” clears a number that has been entered, allowing you to change your input.

The “M” on the input screen lets you capture the amount of time in the memory of the device as the default session time. The amount of time most recently captured in memory will be displayed instead of “0 min” in the time indicator for all future sessions. The default time in memory can be reset to zero or to a different default time at any point, while the input screen is displayed.

Once the correct amount of time is entered, touch the blue start button to begin the session.

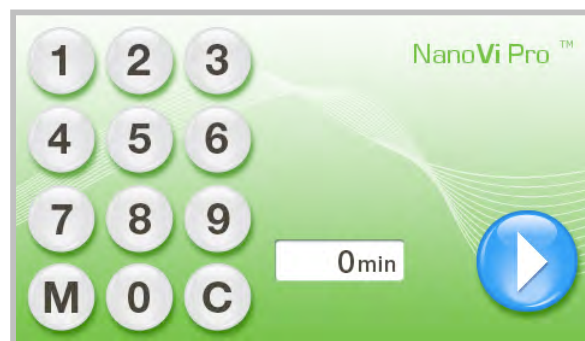


Figure 7.2: Input screen

Figure 7.3 shows the screen when the session is in progress. The digital clock counts down the minutes and seconds remaining in the session. The rotating dots to the left indicate that a session is in progress.

The pause button allows you to interrupt a session (Figure 7.4). Pressing the start button restarts a paused session. If a session has not been restarted within 15 minutes, the device will automatically turn off.

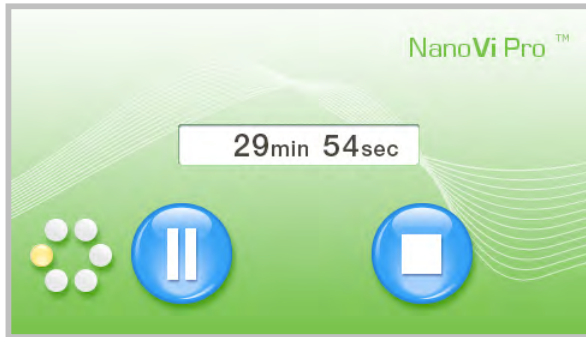


Figure 7.3: Session in progress screen

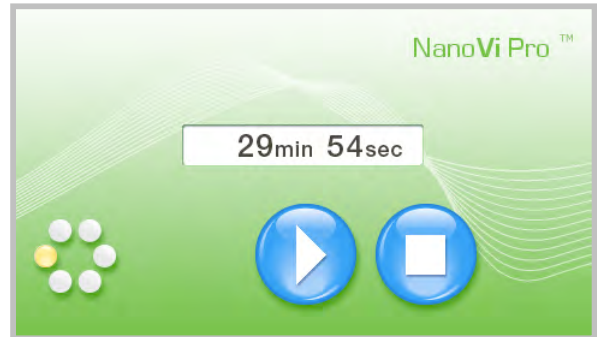


Figure 7.4: Paused session screen

Sessions can be stopped at any time by pressing the stop button. Stopping the session takes you back to the initial entry screen shown in Figure 7.2.

8 Operating in SmartCard Mode

SmartCard mode is available in the NanoVi Exo™ and NanoVi Pro™ devices, not the Eco device. Skip to section 9 if you have a NanoVi Eco™ device.

Insert SmartCards with the arrow showing on the top of the card pointing into the device. The metallic chip must be facing down for the card to work.

Two types of SmartCard are used to operate the device. The Owner Card is used to put the device in SmartCard mode, to program preferences, and to load User Cards with minutes. The User Card is used to operate the device when it is in SmartCard mode. A 4-digit code is printed on the Owner and User Cards that come with the device. This 4-digit code is unique and specific to the device it comes with. The User Cards will only work with the device that was used to program them.

8.1 Owner Card

The owner card can be inserted any time when the device is turned on. It overrides the current functions and presents the administrative screen shown in Figure 8.1. The Owner Card has three basic functions: 1) set preferences on the device, 2) set the operation mode of the device, and 3) program User Cards. Each of these functions is described below. The Owner Card administration screen also shows the rent time (number of minutes of use) and allows you to reset the rent time by pressing the circular arrow at the bottom of the screen.

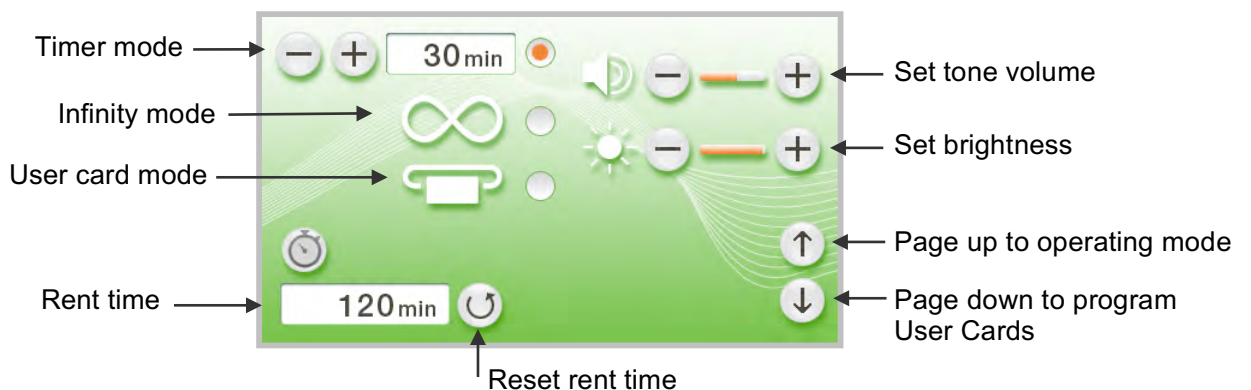


Figure 8.1: Owner Card administrative screen

1) Setting Preferences

Adjust the volume of the tone that sounds when you touch the screen by touching the + or – symbol. Repeatedly touching the – symbol will reduce the volume until the sound is turned off completely.

Adjust the brightness of the screen by touching the appropriate + or – symbols. It is not possible to turn the screen off completely.

2) Setting Operation Mode

The Owner Card administrative screen allows you to set the operation mode of the Exo or Pro device. It can be operated in four different ways: timer mode, infinity mode, User Card timer mode, and User Card session mode. These options are described below.

1. Timer mode – does not require a User Card, the device operates as described in Section 7, Operating in Standard Mode. To select this mode touch the top white button so that a dot appears, as shown to the right.



2. Infinity mode - does not require a User Card and the device remains on, as indicated by the infinity symbol. Figure 8.2 shows the start screen if the device is configured for infinity mode. Figure 8.3 shows the screen displayed during a session in infinity mode. The timer counts up instead of down in infinity mode. Touch the middle button to select infinity mode.


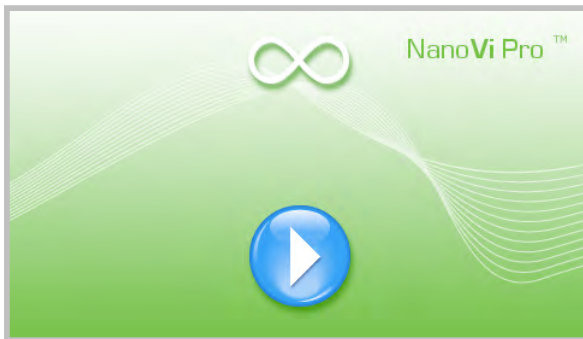


Figure 8.2: Infinity mode start screen



Figure 8.3: Infinity mode session screen

3. User Card timer mode – requires a User Card and allows the user to enter the session time. Select the SmartCard option by touching the bottom button.

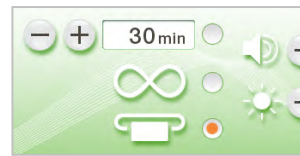

4. User Card session mode - requires a User Card and has a predetermined session time. Select both timer mode and User Card session mode to configure the device in User Card



session mode. Enter the desired session time by pressing the plus and minus arrows of timer mode. Select both the top and bottom buttons for this option.

Once you have selected one of the four operation modes listed above, press the page up arrow in the lower right corner of the Owner Card administration screen. The device goes to the operating mode that was selected and the owner card can be removed.

Selecting the page down arrow in the lower right of the Owner Card screen will take you to the screen for programming User Cards, shown below.

3) Programming User Cards

The screen shown in Figure 8.4 indicates that you should insert a User Card to be loaded with minutes. Remove the owner card and insert the first User Card to be loaded. To return to the Owner Card screen press the page up arrow on the right.



Figure 8.4: Insert User Card for Loading

When the User Card is inserted, the screen shown in Figure 8.5 is displayed. The number of minutes on the card can be seen at the top, above the SmartCard symbol. Selecting the + or – before entering the number of minutes through the touch screen, lets you add or subtract minutes on the card. Minutes that were already on the card can be reduced or eliminated. Once the desired number of minutes shows in the bottom display, press the load card button to load the User Card. Remove the User Card and insert the next one, if you are loading multiple User Cards.

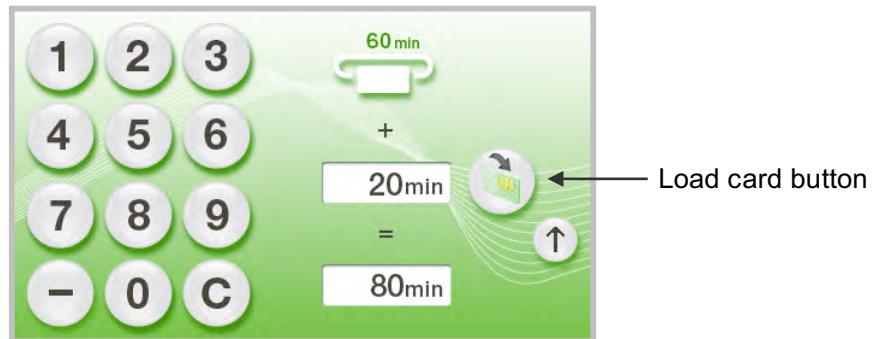


Figure 8.5: Loading User Card

After User Cards are loaded, you can press the page up arrow to return to the owner screen. Pressing the up arrow one more time will take you to the mode that was selected.

If the device has previously been set to require a User Card, the screen shown below in Figure 8.6 will appear after the initial start up screen. The Owner Card can be inserted to administer the device, or the User Card can be inserted to run the device.

8.2 User Card

The screen below is displayed when a User Card is required. A valid User Card, or an Owner Card, must be inserted to operate the device.

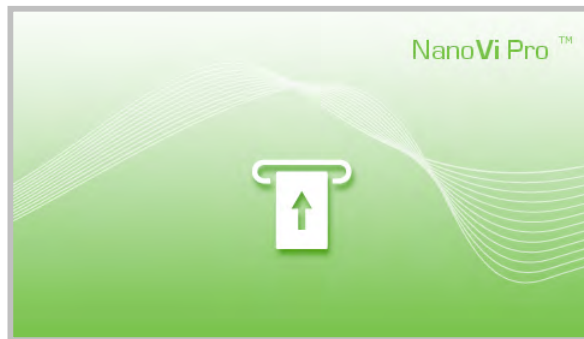


Figure 8.6: SmartCard mode

Timer Mode

The screen shown in Figure 8.7 is displayed when the NanoVi Exo™ or Pro device is configured in User Card timer mode. The SmartCard symbol shows a User Card is inserted. The card time shows the number of minutes remaining on the User Card. The session time display shows the number of minutes entered as the default session time.

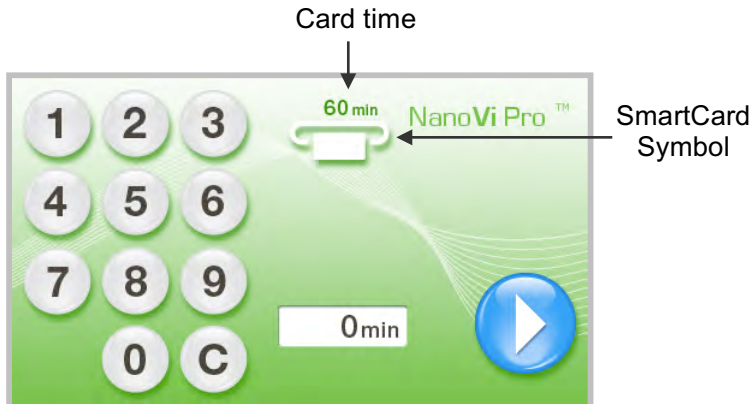


Figure 8.7: User Card timer mode

The session time display shows 0 min, the desired session time must be input through the touch screen. After entering the time, press the start button. The session time will count down and minutes will be deducted from the card.

User Card sessions can be stopped at any time by pressing the stop button. Stopping the session takes you back to the initial entry screen shown in Figure 8.3. Pausing or stopping a session does not affect the number of minutes left on the card.

Session Mode

The device can be set up with a predetermined session time. In this case the session time shows and no keyboard is visible (Figure 8.8). In the example below the session time is 30 minutes and the user has 60 minutes left on their card. Although the time cannot be adjusted, it is still possible to pause or stop a session and to restart a paused session within 15 minutes of touching the pause symbol.

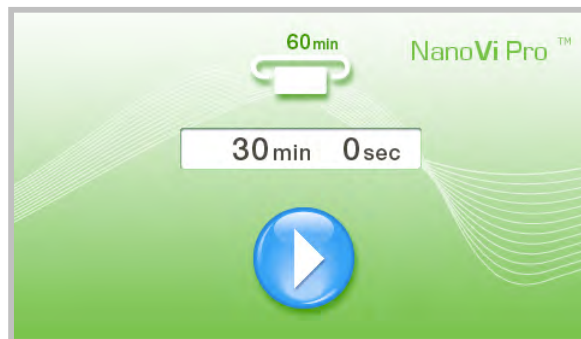


Figure 8.8: SmartCard with predetermined session time

If the User Card is removed at any time while the device is in SmartCard mode, the device will stop operating and display the initial SmartCard mode screen shown in Figure 8.6.

9 Use with Accessories

9.1 Transportation Case

- 1) The Transportation Case is a custom-fitted, hard-shell case.

The case is suitable for checked baggage on airplanes. The outer dimension may allow it to be taken as a carry-on but this depends on the size restrictions for each airline.



- 2) The NanoVi device and necessary accessories fit in custom-designed openings.

The humidifier will leak if water is left in the glass container during transportation. Simply switch the extra glass container with the container that has water and tighten both lids for transport.



The NanoVi™ device can remain in the transportation case during operation.



- 3) The case has two wheels and a pullout / retractable handle.

The case offers the possibility to be locked (lock not included).



Dimensions:

Length: 22.5" (57cm)

Width: 15" (38 cm)

Height: 9" (23 cm)

Weight with device and accessories: 25 lb. (11 kg)



10 Cleaning Instructions

Water in the NanoVi™ device should be changed at the end of each day when used by multiple users. A single user should change the water at least once a week or every five hours of use, whichever comes first.

Device

Clean the outside of the NanoVi™ device with a moist soft cloth, never use more than a mild detergent.



WARNING: Do not clean with solvents. Solvents are aggressive liquids that could corrode and thereby destroy the surface of the device and the touch screen display.

Humidifier (Glass Container, Glass Container Holder and Diffuser)

The humidifier must be removed from the device by pulling it straight up. The glass container is then unscrewed from the top of the humidifier.



WARNING: Do not attempt to unscrew the glass container while the Humidifier is still inserted in the device.

The glass container should be cleaned then rinsed with distilled, purified or osmotic water. It can be cleaned in a dishwasher but should be rinsed with distilled, purified or osmotic water. The diffuser should be rinsed with distilled, purified or osmotic water. It cannot be cleaned using a dishwasher.

If water residue (such as calcareous deposits) is detected on the diffuser, it should be replaced. Contact information for reordering can be found in section 18.



WARNING: Never rinse the inside of the tubes of the humidifier with liquid.



WARNING: Cleaning solution may be harmful and should not be used.

11 Maintenance

The NanoVi™ device requires no special maintenance.

12 Storage

For long-term storage prepare the NanoVi™ device as follows:

1. Remove the plug from the power adapter cable.
2. Disconnect the main DC power transformer from the electrical outlet.
3. Remove the humidifier from the back of the device and empty the water.
4. Clean all parts according to Section 10.
5. Place cleaned device and accessories in their original boxes.
6. Place sealed box in a dry, safe place that is free from the possibility of accidentally falling.

13 Troubleshooting

13.1 Normal Operation

As soon as the NanoVi™ device starts operation, the air pump is switched on and the glass container is illuminated. At the same time the water starts to bubble and a humming from the air pump can be heard.

If the pump is not humming and the water in the humidifier is not bubbling, the air pump is not working.

If the pump is humming but the water in the container is not bubbling, the humidifier has not been correctly inserted into the device. Reseating the connection may resolve this problem. It is also possible that the glass container is not tightly screwed into the glass container holder. Note Figure 5.2 to see how the connection should be made.

If the pump creates little or no airflow, the effectiveness of the device is compromised. Please refer to the error codes below or contact customer support.

13.2 Errors

If an error occurs the error screen shown in Figure 13.1 is displayed. Note the error code number so that you can look it up in the table below. A telephone number is also displayed so that you can contact customer support.

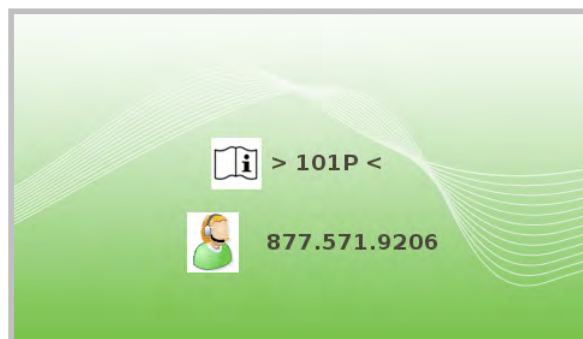


Figure 13.1 Error screen

Error codes are below and should be given to customer support when you call. Use the number of the error message screen to reach technical support for the NanoVi™ device.

Code	Error Message
101P	Pump error
102A	Excitation unit error
103L	Lamp error
104F	Fan error

Table 13.1 Lookup table for error codes

14 Product Specifications and Registrations

14.1 Technical Specifications

	NanoVi Eco™ with Flex-Arm	NanoVi Pro™ with Flex-Arm	NanoVi Exo™
Article Number:	4650-00	4800-00	4900-00
Recommended application time per Recommended frequency of sessions:	60 minutes or more 3 x per week or more	30 minutes or more 3 x per week or more	15 minutes or more 3 x per week or more
Output performance:	100%	200% (Twice the output of the Eco)	400% (Twice the output of the Pro)
Minimum lifespan: Minimum # of sessions per lifespan:	10,000 hours = 600,000 minutes 10,000 sessions of 60 minutes	10,000 hours = 600,000 minutes 20,000 sessions of 30 minutes	10,000 hours = 600,000 minutes 40,000 sessions of 15 minutes
Smartcard system: - Owner Card , pre-programmed at factory. - User Card programmed with device itself and only works on the device it was programmed with.	No	Yes: - Owner Card for selecting the Operation Mode - User Card programmable for up to 9,999 minutes	Yes: - Owner Card for selecting the Operation Mode - User Card programmable for up to 9,999 minutes
Standard mode - Timer Mode:	Yes , enter application time in minutes on the touch screen.	Yes , enter application time in minutes on the touch screen.	Yes , enter application time in minutes on the touch screen.
Mode with Smartcard - Timer Mode: - Session Mode: - Infinity Mode:	No No No	Yes , used application time gets deducted from the User Card. Yes , session minutes deducted from User Card. Yes	Yes , used application time gets deducted from the User Card. Yes , session minutes deducted from User Card. Yes
Option for grouping multiple devices: (With Smartcard System only)	No	Yes , User Card can be used for any device in the group.	Yes , User Card can be used for any device in the group.
Remote controlled illumination of water: Illumination effects:	16 Colors & off Solid, flash, strobe, fade, smooth	16 Colors & off Solid, flash, strobe, fade, smooth	16 Colors & off Solid, flash, strobe, fade, smooth
Excitation units / excitation elements: Spectral emission / max power:	1 / 6 1,100 – 1,300 nm. / 6 x 700 pW	2 / 12 1,100 – 1,300 nm. / 12 x 700 pW	4 / 24 1,100 – 1,300 nm / 24 x 700 pW
Dimensions (w x l x h): Weight:	12" x 11" x 9" (31 x 28 x 23 cm) 8.5 lb. (3.9 kg)	12" x 11" x 9" (31 x 28 x 23 cm) 9.0 lb. (4.1 kg)	12" x 11" x 9" (31 x 28 x 23 cm) 9.5 lb. (4.3 kg)
Silver antimicrobial tubing: Amount of distilled water for operation:	Yes, after humidification unit 8.5 fl oz. (250 ml)	Yes, after humidification unit 8.5 fl oz. (250 ml)	Yes, after humidification unit 8.5 fl oz. (250 ml)
Display: Volume and brightness adjustment:	Touch Screen LCD, color 1 factory setting	Touch Screen LCD, color 8 individual settings	Touch Screen LCD, color 8 individual settings
Pumps: Check valve: Air intake and output:	2 No 0.141 CFM (4.0 liters per minute)	2 Yes 0.141 CFM (4.0 liters per minute)	2 Yes 0.141 CFM (4.0 liters per minute)
Components automatically tested for function:	Pumps, excitation elements, cooling fan, illumination lamp	Pumps, excitation elements, cooling fan, illumination lamp	Pumps, excitation elements, cooling fan, illumination lamp
Service check: Warranty:	Not Required, self testing 2 Years	Not Required, self testing 2 Years	Not Required, self testing 2 Years

Necessary Parts

Glass Container:	Glass
Humidifier unit / holder for Glass Container:	Aluminum
Owner Smartcard for NanoVi Pro and NanoVi Exo:	Pre-programmed to choose the operation mode
User Smartcards for NanoVi Pro and NanoVi Exo:	Programmable for up to 9,999 minutes
Power Supply Input / Output:	100 - 240V AC / 12V DC, 4A
Power Cord (US, UK, EU or AUS):	6 ½ ft. (2 m)
Remote control for color settings:	Includes battery: 3V Type: CR2025
User Manual / Concise User Manual:	Available in different languages

Consumables

Diffuser for Humidifier:	Replace once a year
Paper tube used with Flex-Arm:	White medical paper tubes
Nasal cannulas:	1 ft. (0.3 m) Latex free material
User Smartcards for NanoVi Pro and NanoVi Exo:	Programmable for up to 9,999 minutes
Battery for remote control for color:	3V Type: CR2025

14.2 Product Registrations

NanoVi™, NanoVi Eco™, NanoVi Pro™, and NanoVi Exo™ devices are registered with the United States Food and Drug Administration (FDA).

FDA Device Listing number: D097353

FDA Facility Registration number: 3004152208

All NanoVi™ devices carry the C€ mark represented in the declaration below.

EC Declaration of Conformity

We, the undersigned,

Manufacturer	Eng3 Corporation
Address, City	2234 Eastlake Ave E, Seattle, WA 98102
Country	USA
Phone number	US-206-525 0227
Fax number/e-mail	US-425-650 7171/ customer.care@eng3corp.com
Authorized representative in Europe, Address, City, Country	DFE Consulting, Zum Hahnenberg 8a, 51519 Odenthal, Germany, Fa. Müller Medizinische Labormesstechnik Gmbh, Güpferlingstrasse 11, 1170 Vienna, Austria,

certify and declare under our sole responsibility that the following apparatus:

Description	Wellness Device
Manufacturer	Eng3 Corporation, Seattle, USA
Brand	NanoVi
Identification	NanoVi, NanoVi Eco, NanoVi Pro, NanoVi Exo
Restrictive use	Professional use and Home use

conforms with the essential requirements of the **EMC Directive 2014/30/EU** and **General Product Safety Directive 2001/95/EC**, based on the following specifications applied:

EN 55014-1:2006 + A1:2009 + A2:2011
EN 55014-2:1997 + Corrigendum 1997 + A1:2001 + A2:2008
EN 55015:2013

and therefore complies with the essential requirements and provisions of the EMC Directive.

Name	Hans J. Eng
Position of person binding	President / CEO
the manufacturer	Eng3 Corporation
or his authorized representative	---
Date	August 18, 2015
Signature	

15 Warranty

Devices manufactured or distributed by Eng3 Corporation carries a warranty, covering materials and workmanship, for a period of two years from the date of shipment, except for certain disposable products with stated warranties with different durations. Eng3 reserves the right to perform warranty service(s) at its factory, at an authorized repair station, or at the customer's facility.

Eng3's obligations under this warranty are limited to repairs, or at Eng3's option, replacement of any defective parts or of equipment without charge, if defects occur during normal usage.

Claims for damages during shipment must be filed promptly with the transportation company. All correspondence concerning the equipment must specify both the model name and number and the serial number as it appears on the device.

Improper use, mishandling, tampering with, or operation of the device without following specific operating instructions will void the warranty and release Eng3 from any further warranty obligations.

The actual warranty, outlining all terms and conditions, is included in the paperwork for the NanoVi™ device.



WARNING: Warranty immediately revoked if the device is opened or repaired by unauthorized personnel.



WARNING: Warranty immediately revoked if any accessories other than those recommended have been used.

Service Department
For factory repair service call:
1.206.525.0227
Facsimile: 425.650.7171

16 Service Policy

Eng3 Corporation will provide warranty service support to its customers within 48 hours of receiving a telephone request for technical support. This 48-hour period begins once a service request is placed through the Factory Technical Support Department in Seattle, Washington. Eng3 provides factory direct technical support to its customers through a technical support group located in Seattle, Washington. All Technical Support for Eng3 products is provided “Factory Direct”.

Eng3 provides technical support by telephone number: 1.877.571.9206 or email address: customer.care@eng3corp.com. It is suggested that any person calling in for technical support have the inoperative equipment available for preliminary troubleshooting as well as product identification. Eng3 reserves the right to repair or replace any product found to be defective during the warranty period. Repair may be provided in the form of replacement or exchange of parts or accessories, on-site technical repair assistance or complete system exchanges. Repairs provided due to product abuse or misuse will be considered “non-warranty” and invoiced at the prevailing service rate. Any replaced defective material should be returned to Eng3 within 10 days of being provided in order to avoid additional charges. Exchanged material should be returned promptly and directly to Eng3 using the return paperwork and shipping label(s) provided. Transferring return materials to local sales or dealer representative does not absolve the return responsibility.

17 Ordering Parts and Accessories

To order parts and accessories contact your local sales representative or Eng3 Corporation at: (1) 206-525-0227

Complete contact information is found below in Section 18.

18 Contact Information

MANUFACTURER

Eng3 Corporation

2234 Eastlake Avenue E. Ste. A

Seattle, WA 98102

Office phone: (1) 206-525-0227

Fax: (1) 425-650-7171

E-Mail: Info@eng3corp.com

URL: www.eng3corp.com

IMPORTER / REPRESENTATIVE

